


# Measurement 2023\_07\_31-16\_56\_02\_results: Temperature sweep 25.0--30.0 degC @ 55.0 % r.h.

$\Delta\phi(S_{21PKPK})$ : 0.814 °  
 $\Delta|S_{21PKPK}|$ : 0.040 dB

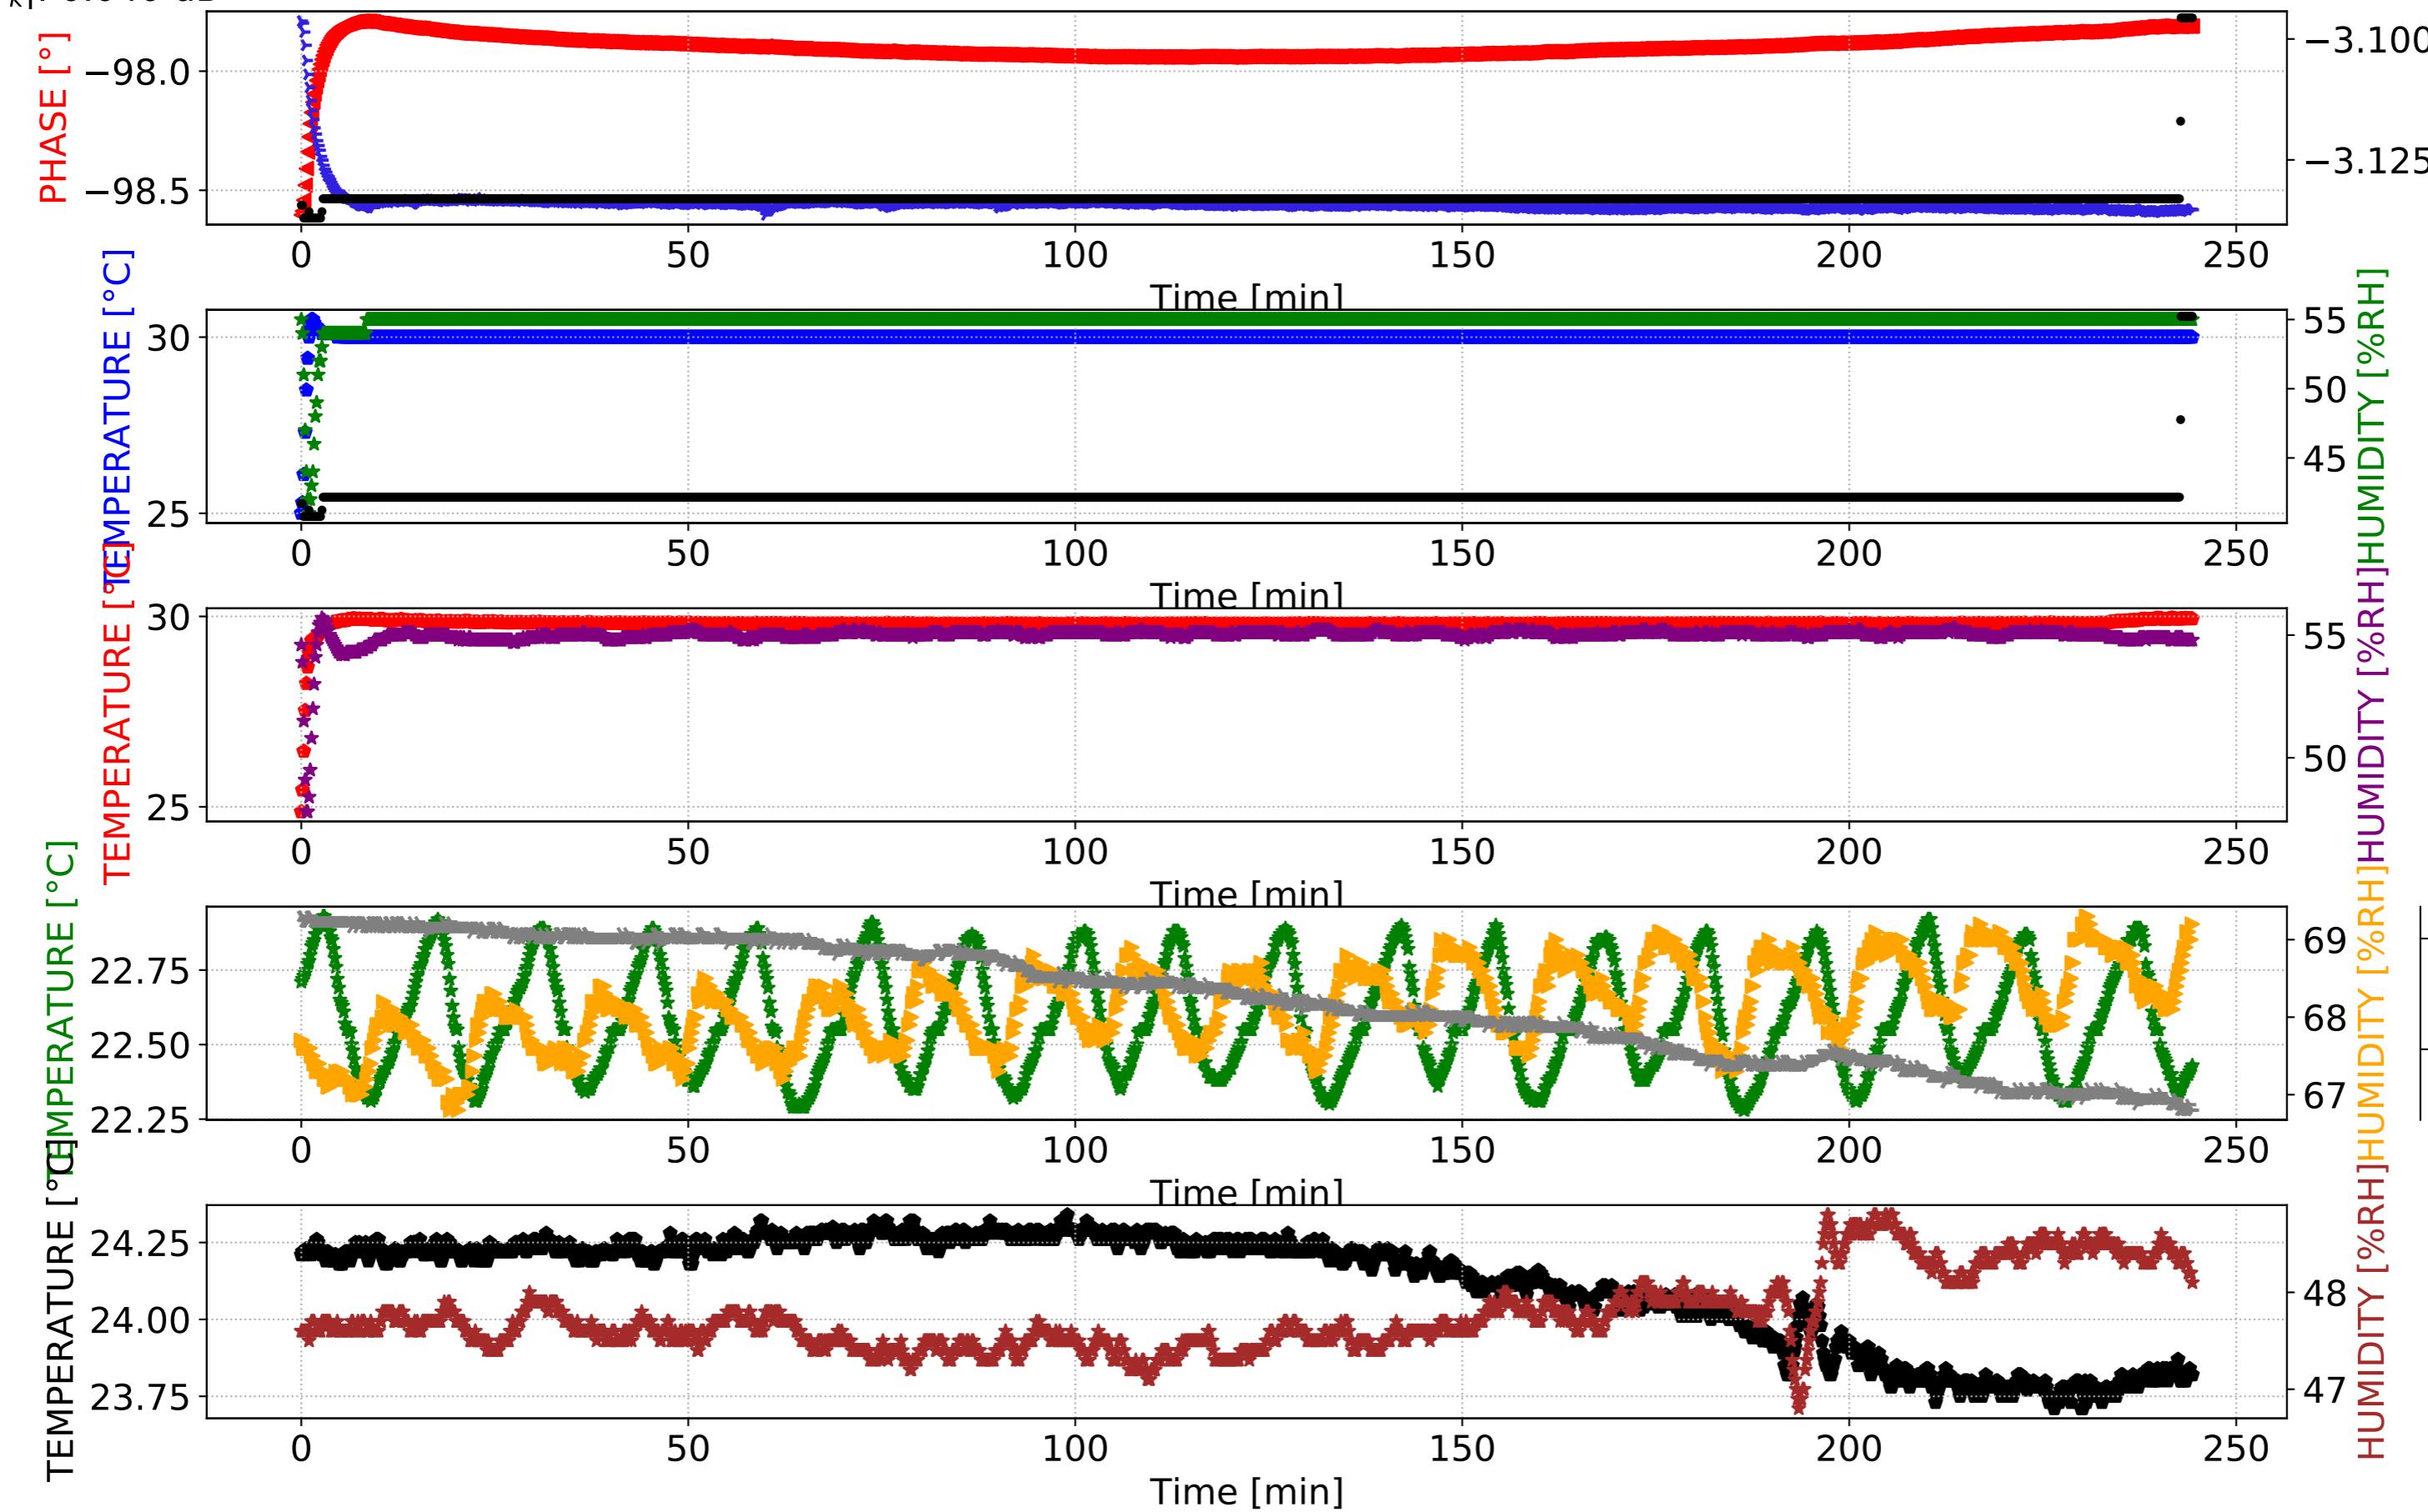

- DUT Phase
- DUT Magnitude
- Equilibrium\_Indicator
- Chamber Temperature
- Chamber Humidity
- Equilibrium\_Indicator
- DUT temperature
- DUT humidity
- room temperature
- room humidity
- air pressure room
- temperature  
almemo sensors  
meas instr cham
- humidity  
almemo sensors  
meas instr cham